
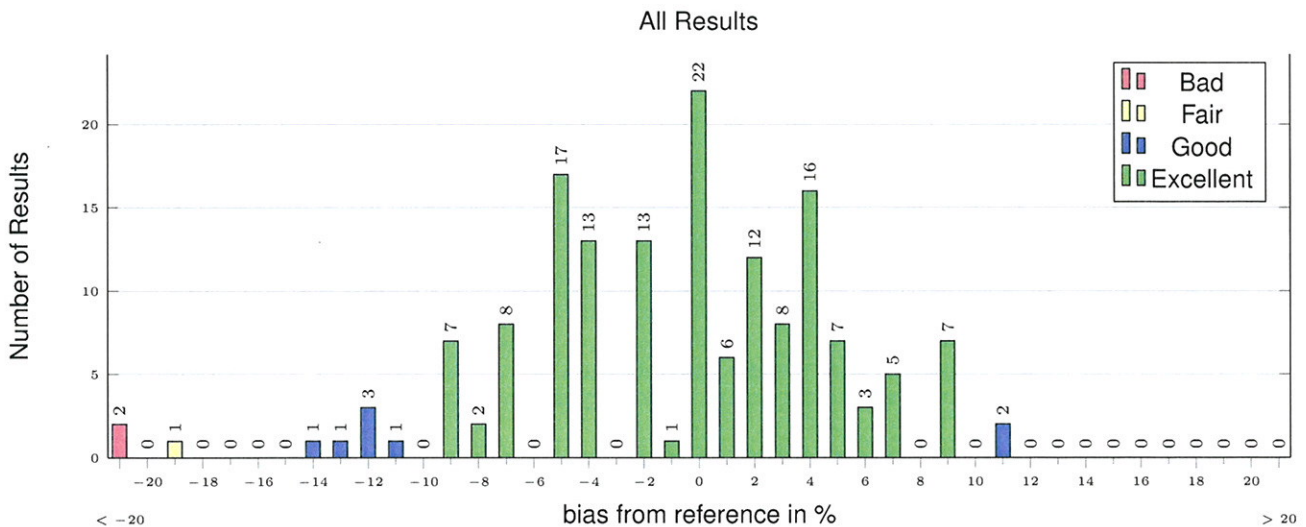


Report Settings

Sample	2081403 (March - 2014)
Lot	2081403
Analyte	Glucose
Field type	Value
Reference	Median per Instrument Type
Calibration	whole_blood

Glucose	My Results	All Results
n	1	158
minimum	5.9	4.2
maximum	5.9	6.3
average	5.9	5.6
median	5.9	5.7
SD	-	0.3
CV	-	6.2%
Est. Uncertainty	0.00	0.03

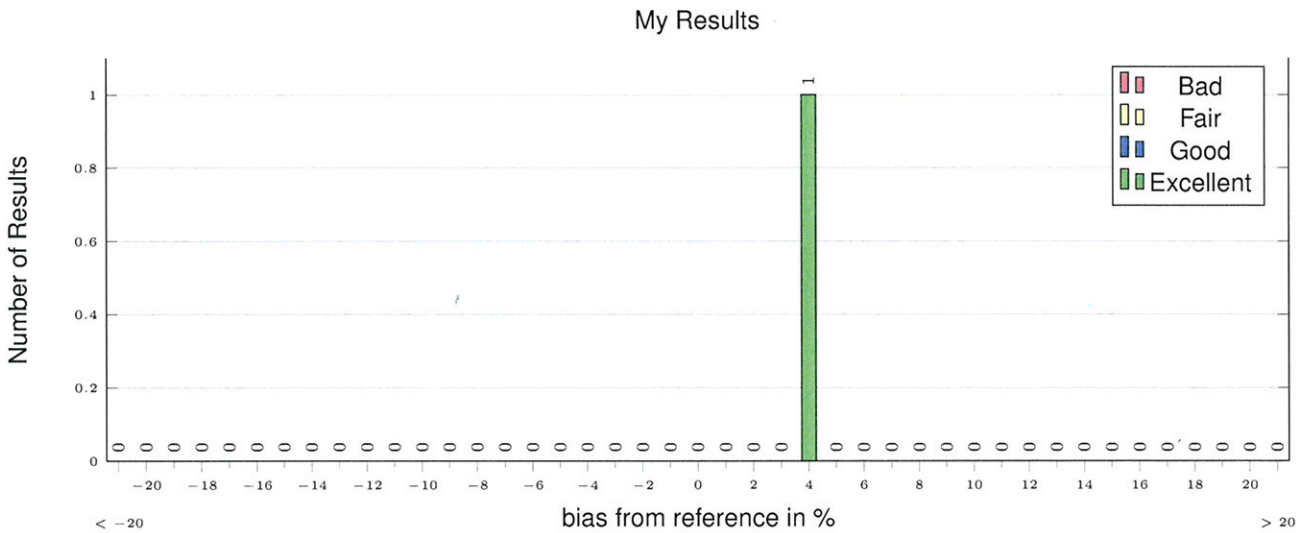

Instrument Type	n	median	SD
HemoCue Glucose	158	5.7	0.3